


Coronis Uniti

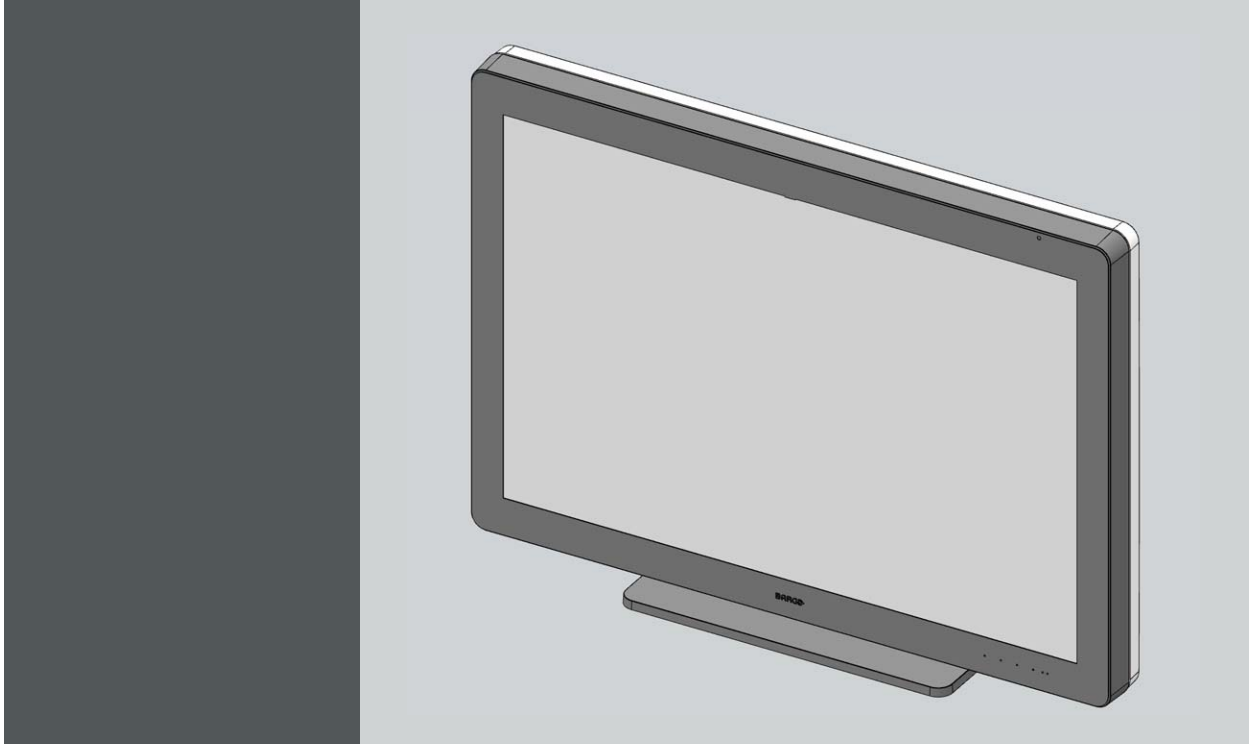

User Guide

MDMC-12133

Barco nv

President Kennedypark 35, 8500 Kortrijk, Belgium

Phone: +32 56.23.32.11

Fax: +32 56.26.22.62

Support: www.barco.com/esupport

Visit us at the web: www.barco.com

Printed in Belgium

TABLE OF CONTENTS

1. Welcome!	3
1.1 About the product	3
1.2 What's in the box	3
2. Parts, controls and connectors	5
2.1 Display front view	5
2.2 Display rear view	6
2.3 Accessories	7
3. Display installation	9
3.1 Removing the connector compartment cover	9
3.2 Unlocking the tilt mechanism	10
3.3 Unlocking the height mechanism	10
3.4 Adjusting the display position	11
3.5 Connecting the signal cables	12
3.6 Connecting the power cable	14
3.7 Mounting the film clip	15
3.8 Mounting the MultiTouchPad	16
3.9 Routing the cables & Reattach the connector compartment cover	17
3.10 Fixation of the foot on the desk	18
3.11 VESA-mount installation	19
3.12 First time starting up	22
4. Daily operation	23
4.1 Recommendations for daily operation	23
4.2 Key indicator lights	24
4.3 Standby switching	24
4.4 Bringing up the OSD menus	25
4.5 Navigating through the OSD menus	25
4.6 Overview of the functionality of the Left/Right keys	26
4.7 I-Luminate	27
4.8 Extended display keypad functions	27
4.8.1 I-luminate mode	27
4.8.2 Viewing mode	27
5. Advanced operation	29
5.1 OSD menu language	29
5.2 OSD menu automatic close function	29
5.3 Power status indicator light	29
5.4 Key indicator lights	30
5.5 Power lock function	30
5.6 SoftGlow Task light	30
5.7 SoftGlow Wall light	31
5.8 DPMS mode	31
5.9 Hibernate	32
5.10 I-Luminate default mode	32
5.11 I-Luminate film position	33
5.12 Luminance target	33
5.13 Color presets	33
5.14 Color temperature	34
5.15 Color coordinates	34
5.16 Viewing modes	34
5.17 Display functions	35
5.18 Ambient Light Compensation (ALC)	36
5.19 Reading rooms	36
5.20 Continuous ALC	37
5.21 Embedded QA	37
5.21.1 About Embedded QA	38

5.21.2 DICOM status report	38
5.21.3 DICOM compliance check	39
5.21.4 DICOM calibration	39
5.21.5 Reset DICOM calibration	39
5.21.6 DICOM error threshold	40
5.22 Image scaling	40
5.23 Image source selection modes	40
5.24 Grayscale conversion modes	41
5.25 Input interface standard version	41
5.26 EDID format	42
5.27 EDID timings	42
5.28 Display info	42
5.29 Display status	43
6. Cleaning your display	45
6.1 Cleaning instructions	45
7. Important information	47
7.1 Safety information	47
7.2 Environmental information	48
7.3 Regulatory compliance information	50
7.4 EMC notice	51
7.5 Explanation of symbols	54
7.6 Legal disclaimer	56
7.7 Technical specifications	56
7.8 Open source license information	58

1. WELCOME!

1.1 About the product

Overview

Thank you for choosing this Coronis Uniti!

Coronis Uniti is an ingenious PACS display system designed to enhance flexibility and productivity in diagnostic imaging. Featuring the industry's first 33-inch color LCD that can be used as two seamless heads or one wide-screen display, Coronis Uniti offers you the freedom to organize your workspace just the way you want it. It allows you to read radiology, mammography, and breast tomosynthesis images, side by side on a single diagnostic screen. Coronis Uniti features Barco Optical Glass illuminated by DuraLight Brilliance to provide an exceptional image over your entire field of view. Use the instructions in this guide to install your Coronis Uniti display and discover the productive features and included accessories!



CAUTION: Read all the important safety information before installing and operating your Coronis Uniti. Please refer to the dedicated chapter in this user guide.

1.2 What's in the box

Overview

Your Coronis Uniti comes with:

- this Coronis Uniti user guide
- Quick Installation Sheet
- a system CD
- two DisplayPort cables
- a USB cable
- a set of AC power cords
- an external power supply
- Film clip
- MultiTouchPad

If you ordered a Barco display controller, it's also in the box together with its accessories. A dedicated user guide is available on the system CD.



Keep your original packaging. It is designed for this display and is the ideal protection during transport and storage.

2. PARTS, CONTROLS AND CONNECTORS

2.1 Display front view

Overview

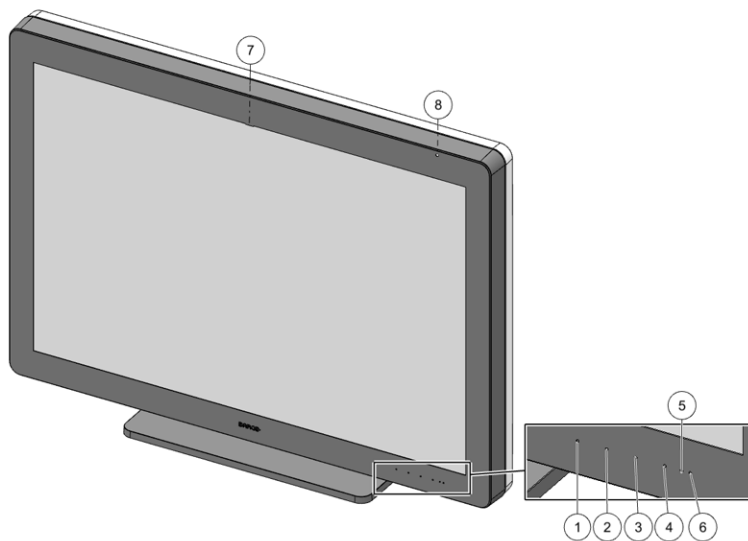


Image 2-1
Front view

- | | |
|---|--|
| ① I-Luminate/Left key | ② Right key |
| ③ Menu key | ④ Standby key |
| ⑤ Power status indicator light (Power On) | ⑥ Power status indicator light (Standby) |
| ⑦ I-Guard | ⑧ Ambient light sensor |

2.2 Display rear view

Connector compartment cover closed

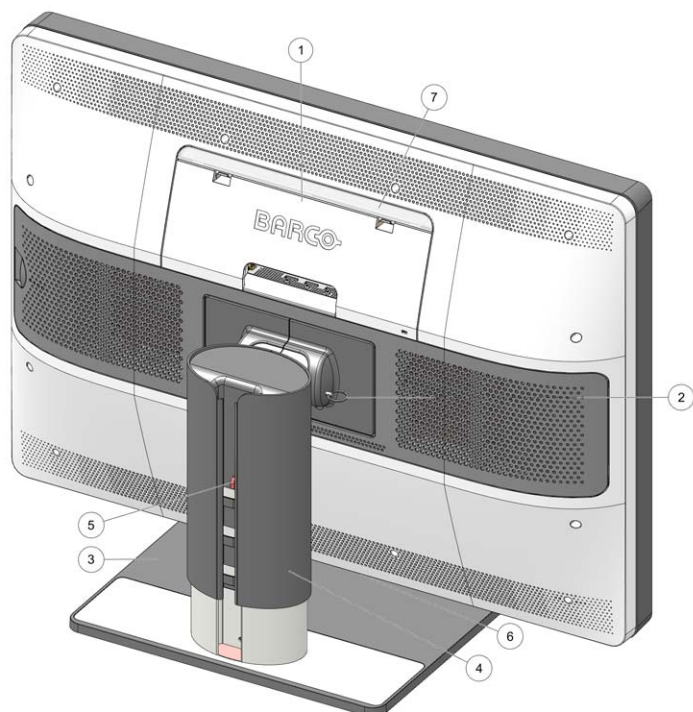


Image 2-2
Rear view with closed connector compartment cover

- | | |
|---|---|
| ① Connector compartment cover | ② Tilt lock pin (only for transportation) |
| ③ Tilt & swivel foot | ④ Cable duct |
| ⑤ Foot lock pin (only for transportation) | ⑥ SoftGlow Task light |
| ⑦ SoftGlow Wall light | |



Store the foot lock pin and tilt lock pin for possible future transportation of the display.

Connector compartment cover open

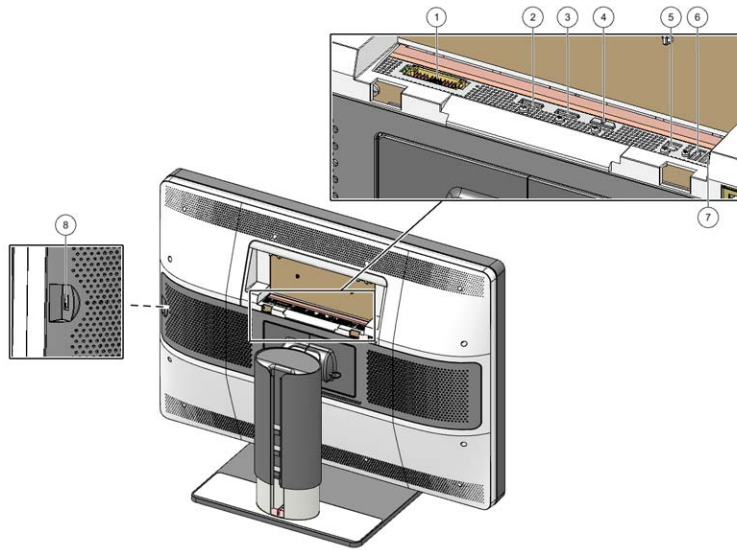


Image 2-3
Rear view with open connector compartment cover

- | | |
|----------------------------|----------------------------|
| ① Power connector | ② Display port connector |
| ③ Display port connector | ④ Not used |
| ⑤ USB upstream connector | ⑥ USB downstream connector |
| ⑦ USB downstream connector | ⑧ USB downstream connector |

2.3 Accessories

Film clip

The film clip can be used to hold a radiological film when using the I-Luminate function as a light box.

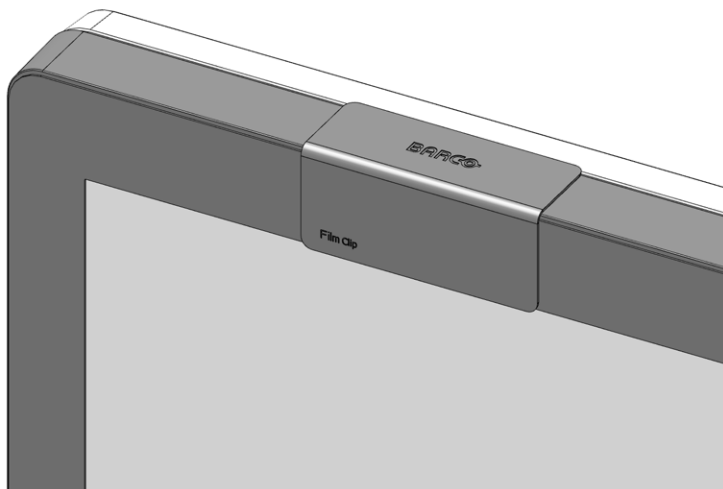


Image 2-4
Film clip

MultiTouchPad

The MultiTouchPad enables and controls SpotView.

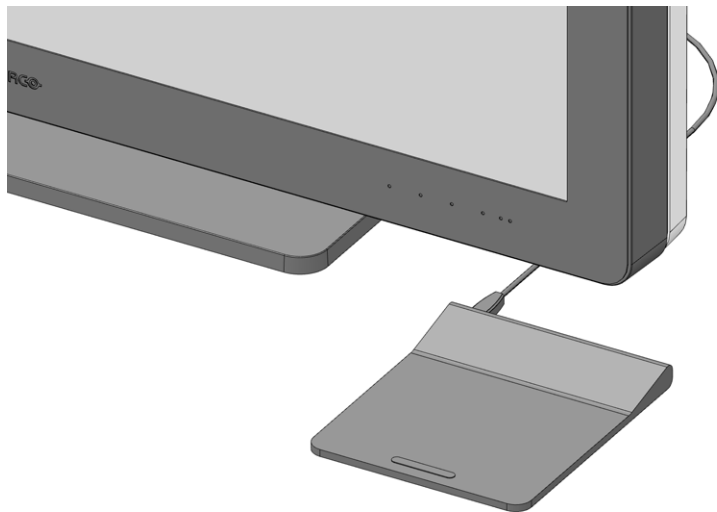


Image 2-5
MultiTouchPad

3. DISPLAY INSTALLATION



Prior to installing your Coronis Uniti and connecting all necessary cables, make sure to have a suitable display controller physically installed in your computer. If you are using a Barco display controller, please consult the user guide delivered with it to do this.

For a list of compatible display controllers, please refer to the latest version of the compatibility matrix available on myBarco.com (myBarco > My Support > Healthcare > Compatibility Matrices > Barco Systems Compatibility Matrices).


3.1 Removing the connector compartment cover



The connector compartment cover should be removed to get access to the connectors.

To remove the connector compartment cover

1. Gently push the two lips on the top of the cover.
2. Pull the top of the cover slightly away from the display and lift the cover upwards.

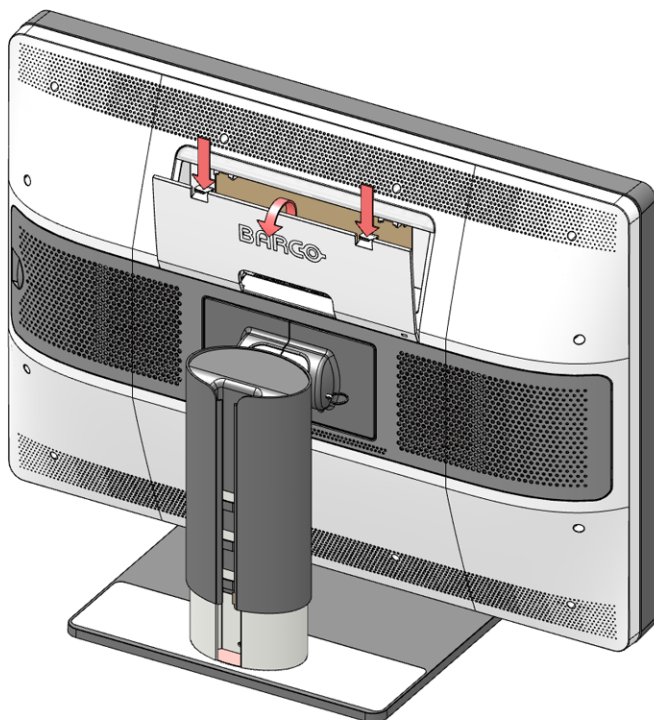

3. Remove the cover.

3.2 Unlocking the tilt mechanism




In the factory, the tilt system in the display stand is locked with a red pin to prevent damage during transportation. You'll have to remove this pin before adjusting your display position.



Push the display against the buffer part to easily remove the pin.

To remove the pin:

1. Position the display with its rear side facing you.
2. Pull out the red pin in the display stand.

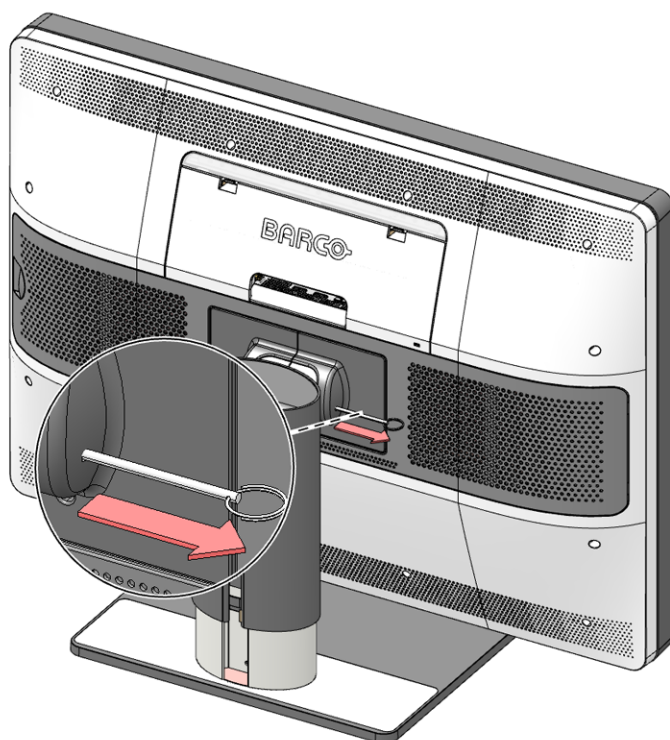

3. Keep the pin in case the display needs to be shipped later.



WARNING: Before transportation of the display, insert the pin in the lock mechanism so that the grey color of the pin isn't visible anymore.


3.3 Unlocking the height mechanism



In the factory, the height-positioning system in the display stand is locked with a red pin to prevent damage during transportation. You'll have to remove this pin before adjusting your display height position.

To remove the pin:

1. Position the display with its rear side facing you.
2. While holding the display panel pushed down, pull out the red pin in the display stand.

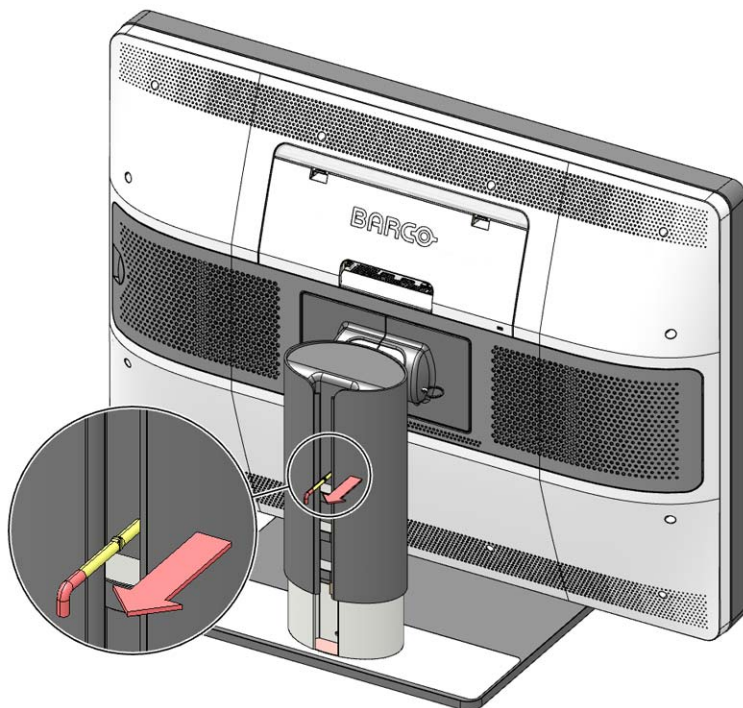

3. Keep the pin in the dedicated hole in case the display needs to be shipped later.



To retain the pin for possible future transportation, insert the short, red end of the pin back into the stand of your display.


3.4 Adjusting the display position



In the factory, the height-positioning and the tilt system in the display stand are locked with red pins to prevent damage during transportation. You'll have to remove both pins before adjusting your display position.

To adjust the display position

1. Remove the tilt lock pin, see "Unlocking the tilt mechanism", page 10.
2. Remove the height lock pin in the display stand, see "Unlocking the height mechanism", page 10.
3. Tilt, swivel, raise and lower the display as desired.

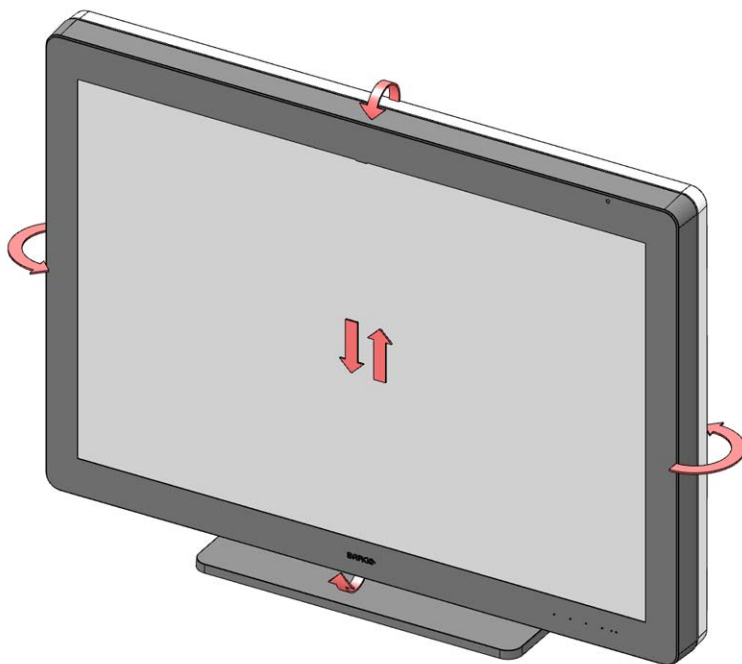

CAUTION: Do not try to pivot your display when attached to the stand. Trying to do so could cause serious damage to your display and its stand.


3.5 Connecting the signal cables




To get access to the connectors, remove the connector compartment cover. See "Removing the connector compartment cover", page 9 .

To connect the signal cables to the display:


1. Connect one head of the display controller to the DisplayPort connector with one of the supplied DisplayPort cables.

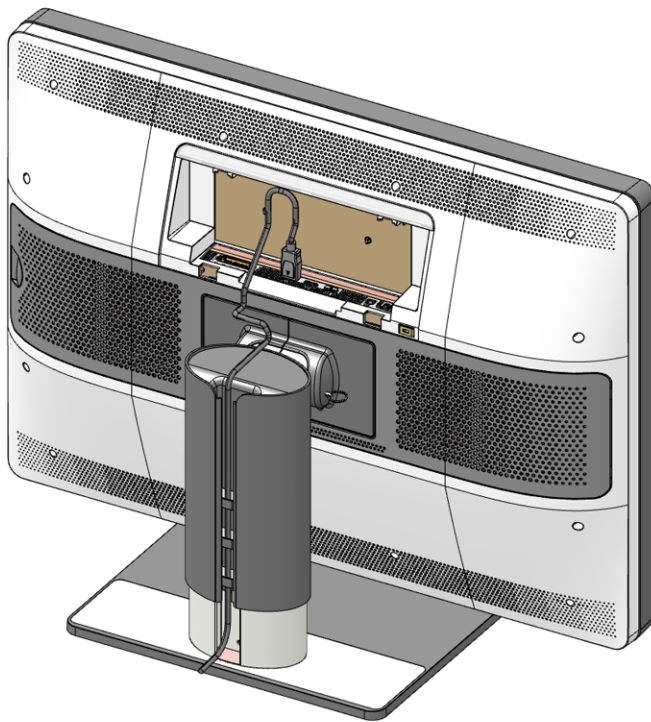

2. Connect another head of the display controller to the other DisplayPort connector with one of the supplied DisplayPort cables.

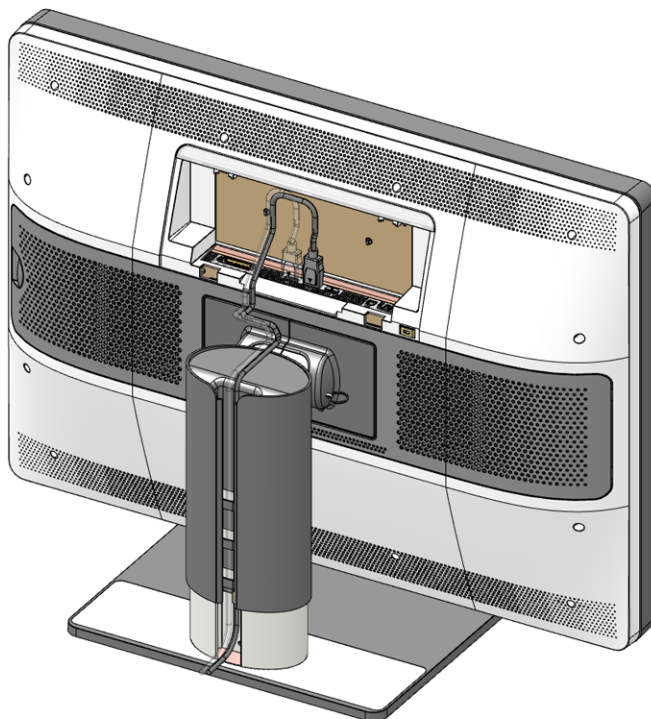

3. Connect a PC USB downstream connector to the display's USB upstream connector by means of the supplied USB 2.0 cable.

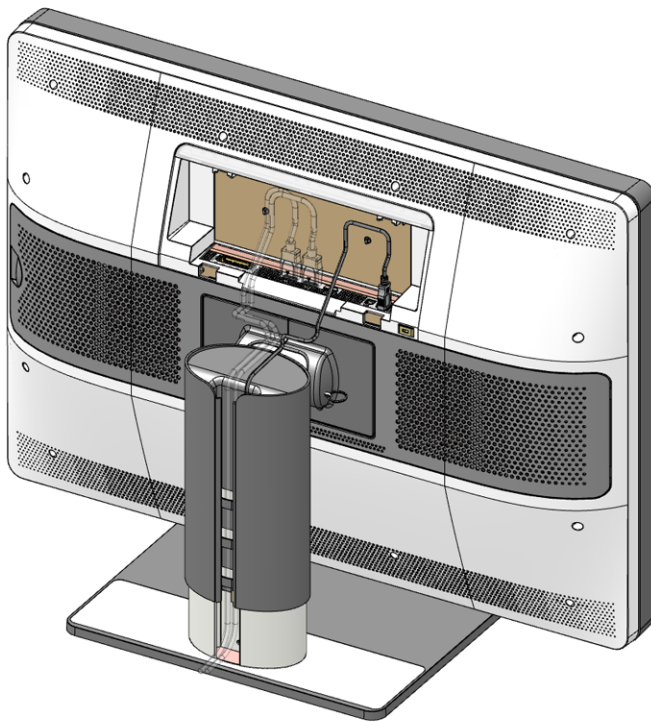


Communication with the display is possible via DisplayPort although it is recommended to use the USB upstream connector for faster communication.

3.6 Connecting the power cable

To connect the power cable to the display:

1. Connect the supplied external DC power supply to the +24 VDC power input of your Coronis Uniti display.

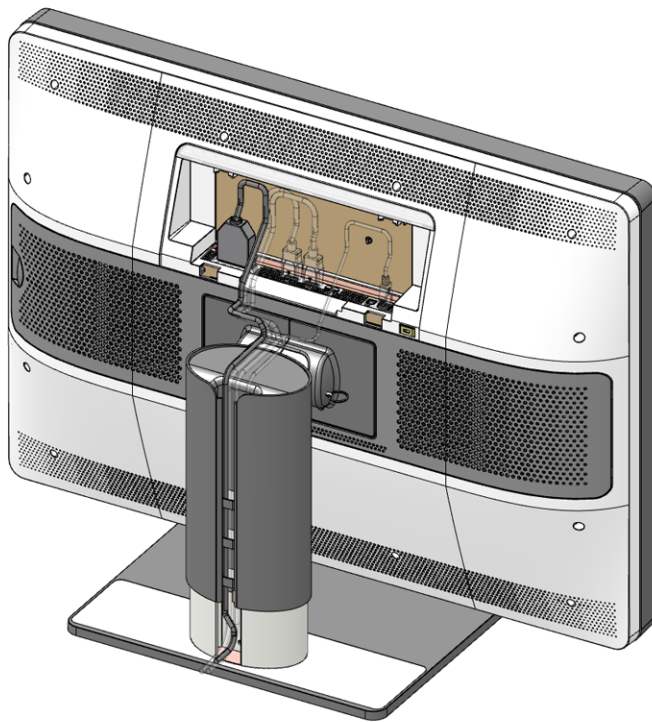

Warning: Fasten the power connector to your display with the screws provided at the sides of the connector.

2. Plug the other end of the external DC power supply into a grounded power outlet by means of the proper power cord delivered in the packaging.




Use the external power supply delivered with your display. If you do not use the correct power supply, the display will not start up.

3.7 Mounting the film clip

To mount the film clip

The film clip can be mounted on the top side of the display.

1. Position the film clip on the top side of the bezel at the desired location (in the middle, left or right).

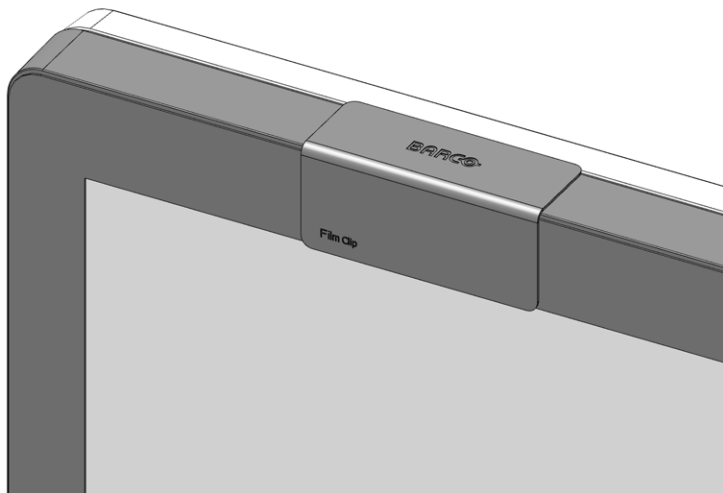


2. To remove the film clip, lift the front end or rear end of the clip.

3.8 Mounting the MultiTouchPad

To mount the MultiTouchPad

1. Connect the MultiTouchPad to one of the USB downstream connectors (using either those found in the cable compartment or on the right side of the display).

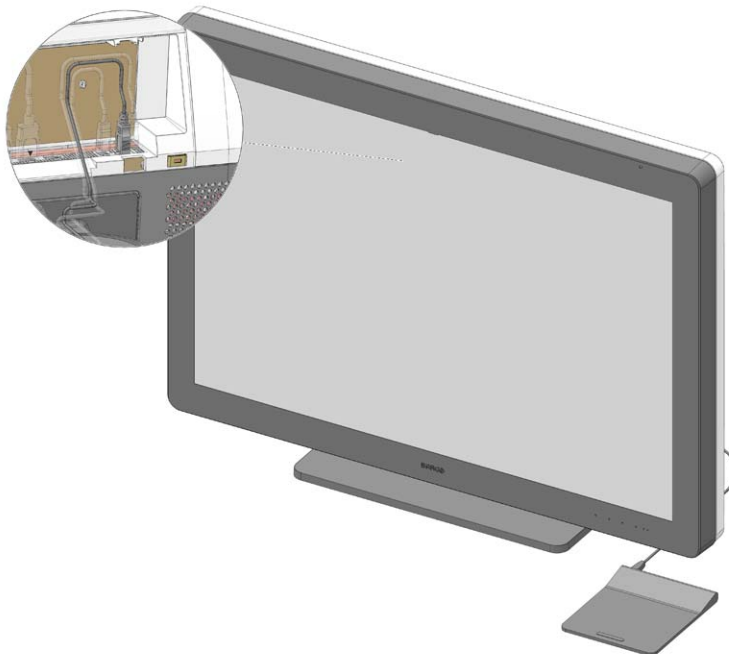


2. With the MultiTouchPad attached and the driver installed, simply press on the MultiTouchPad to move the focus on the SpotView around the display(s). The SpotView vanishes when no finger is pressing on the MultiTouchPad, unless the left side of the MultiTouchPad button is held down.

3.9 Routing the cables & Reattach the connector compartment cover

To route the cables


1. Route all connected cables through the cable routing channel in the stand of your display.

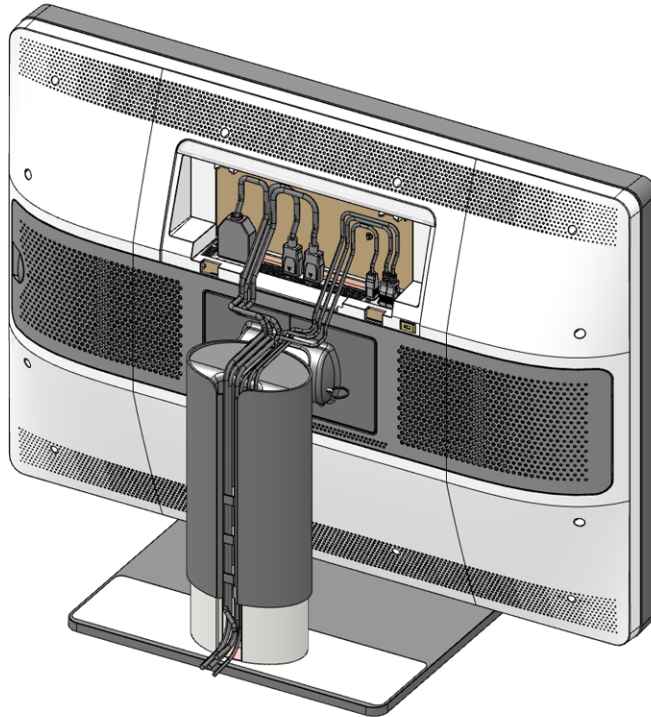

Tip: The cable straps at the inside of the connector compartment allow you to fix the cables for better shielding of the cables.

To reattach the connector compartment cover

1. Reattach the connector compartment cover by sliding the cover's top. You'll hear a "click" sound of the cover's clips when the connector compartment cover is in position.

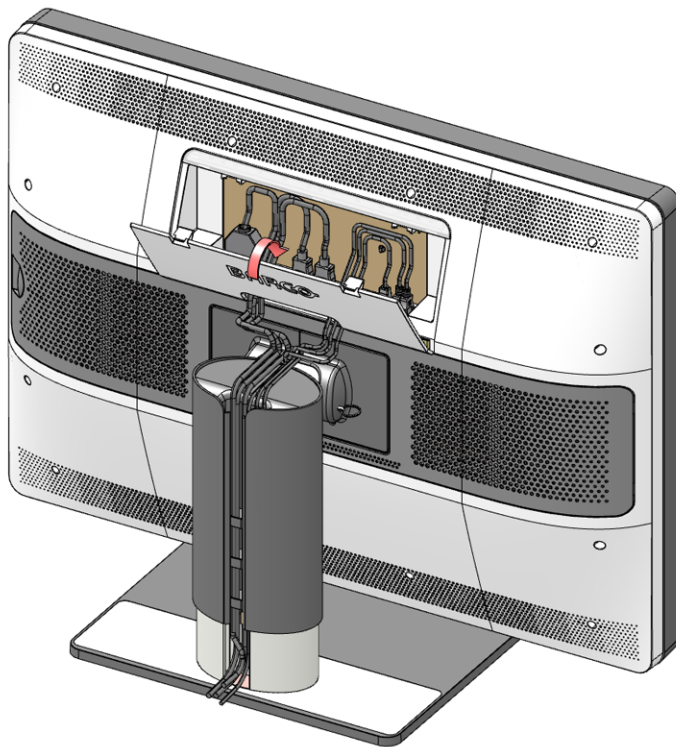


3.10 Fixation of the foot on the desk

Overview

If you would like to attach the Coronis Uniti to a desk, the tilt & swivel foot has 4 screw holes (4x M4) to mount the foot on a desk.

1. Drill four holes in the desk.

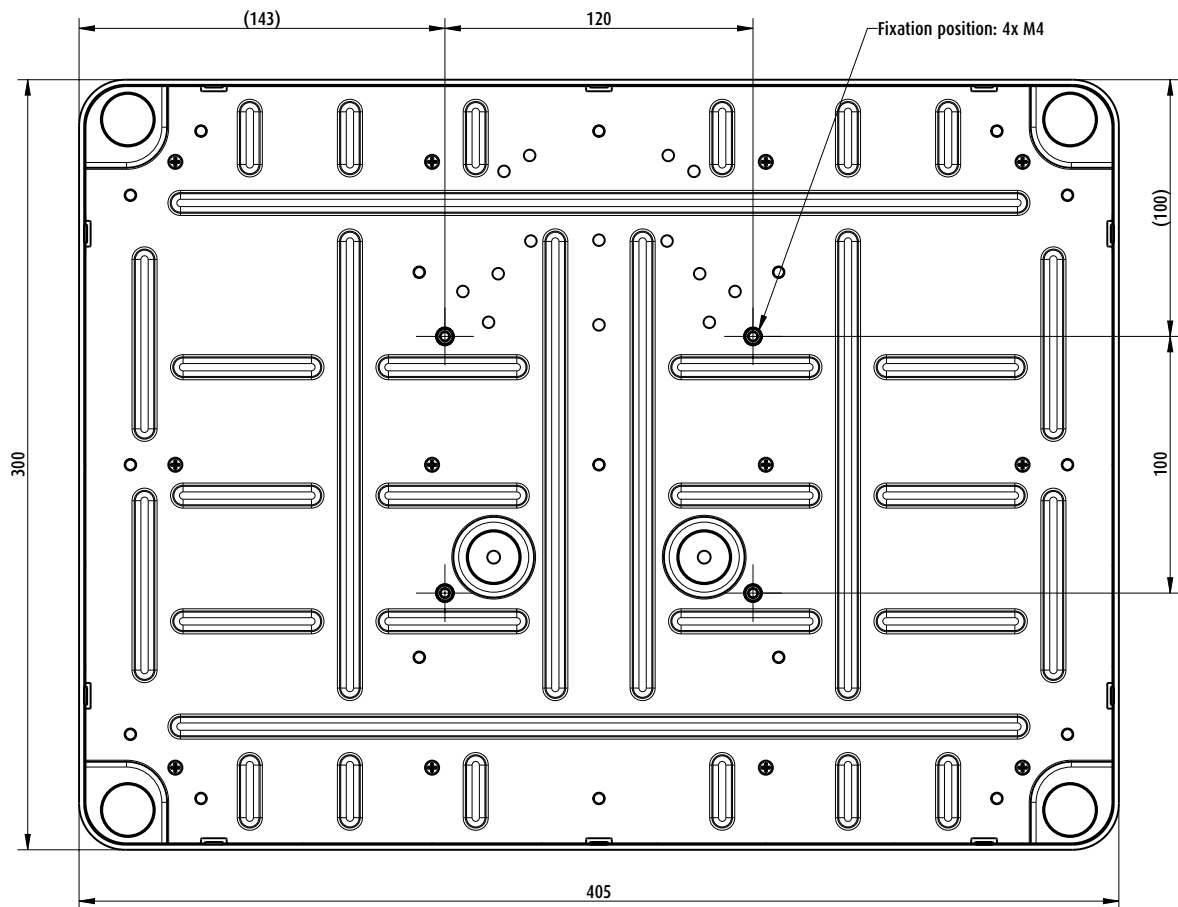

2. Fasten the foot on the desk with 4x M4 screws (length of the screws depending on the depth of the desk).

3.11 VESA-mount installation



CAUTION: Use suitable mounting apparatus to avoid risk of injury.



WARNING: Never move a display attached to an arm by pulling or pushing the display itself. Instead, make sure that the arm is equipped with a VESA approved handle and use this to move the display.

Please refer to the instruction manual of the arm for more information and instructions.



WARNING: Use an arm that is approved by VESA (according to the VESA 200 x 100 mm or VESA 100 x 100 mm standard).

Use an arm that can support the weight of the display. Refer to the technical specifications of this display for the applicable weight.

3. Display installation



CAUTION: You should mount the panel in landscape position. Portrait position is possible but not supported.




WARNING: To avoid muscle strain or back injury, use lifting aids and proper lifting techniques when removing or replacing.

Overview



The panel, standard attached to the tilt & swivel foot, is compatible with the VESA 200 x 100 mm and VESA 100 x 100 mm standard. So it can be used with an arm stand according to the VESA 200 x 100 mm or VESA 100 x 100 mm standard.

Therefore, the tilt & swivel foot must be removed from the panel.


1. Fasten the height mechanism of the foot by putting the red pin in the hole "Unlocking the height mechanism", page 10.
2. Put the display face down on a clean and soft surface. Be careful not to damage the panel screen.
3. Loosen the plastic covers with a cross head screwdriver.

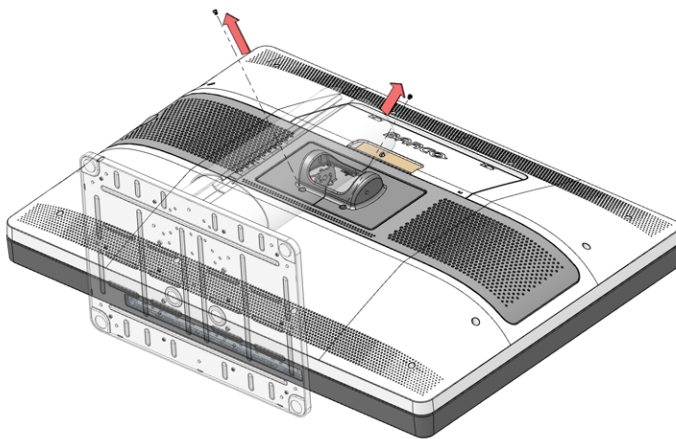

4. Remove the two plastic covers.

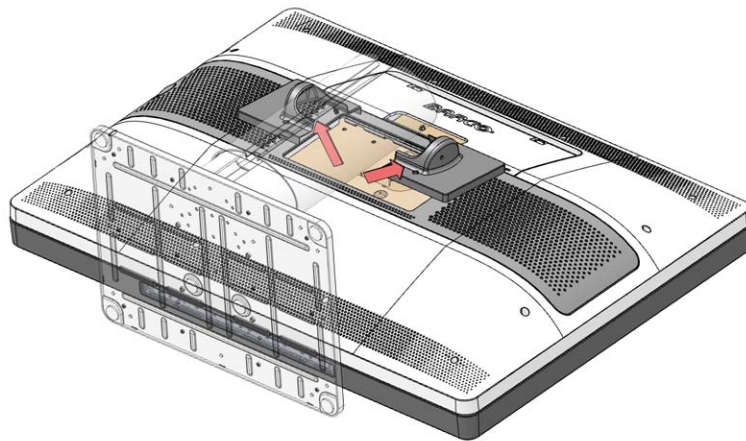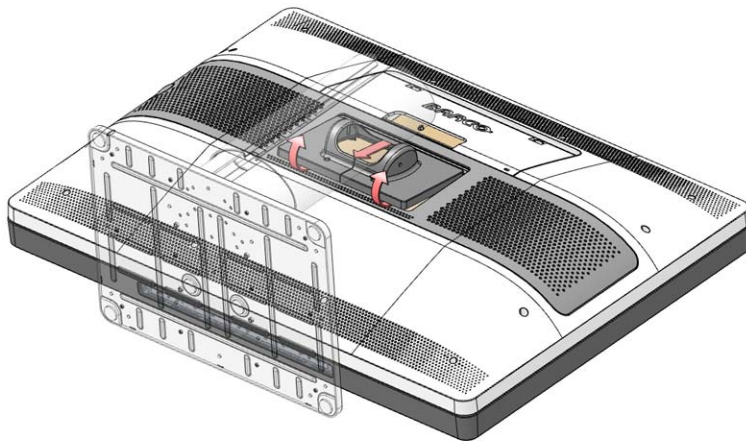


5. Remove the 9 screws fixing the foot while supporting the foot.

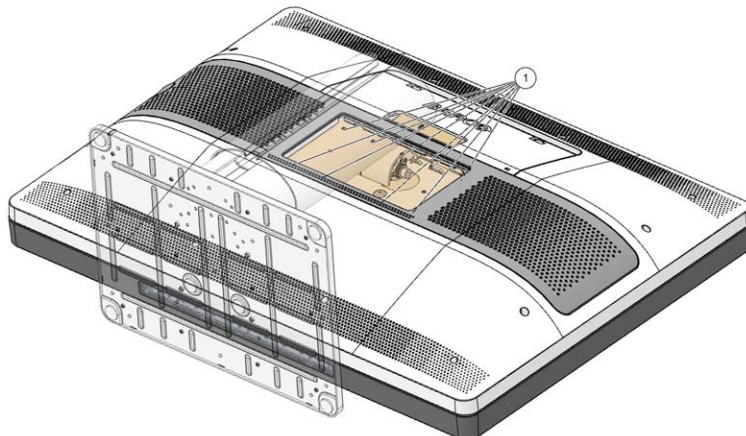

3. Display installation

6. Attach the arm stand **firmly** to the panel using 6 screws M4 x 6 mm for a 200 x 100 mm VESA solution or 4 screws M4 x 6 mm for a 100 x 100 mm VESA solution.

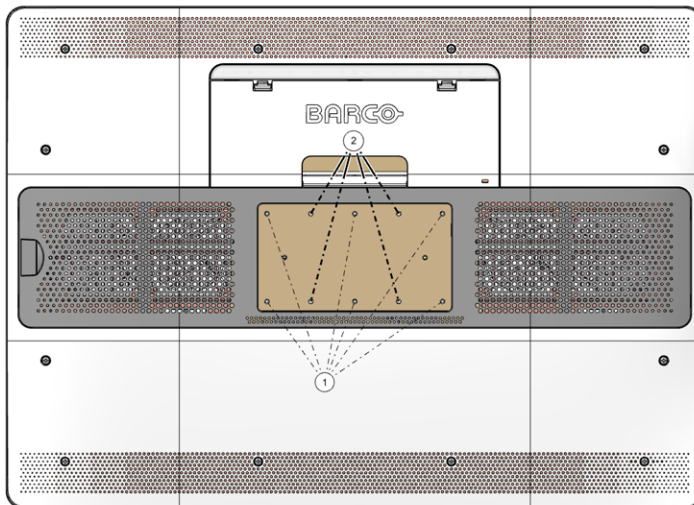

WARNING: Never move a display attached to an arm by pulling or pushing the display itself. Instead, make sure that the arm is equipped with a VESA approved handle and use this to move the display.

Please refer to the instruction manual of the arm for more information and instructions.

3.12 First time starting up

Overview

You are now ready to start up your Coronis Uniti for the first time.

1. Switch on your Coronis Uniti as described in "Standby switching", page 24.
2. Turn on the computer connected to your display.

If you have properly installed your display and display controller, the Windows start-up messages will appear once the boot procedure is finished.



Your Coronis Uniti display will be running in a basic video mode at a default refresh rate when first time starting up. If you are using a Barco display controller, please consult the dedicated user guide available on the system CD to install the drivers, software and documentation. When this is done, your display will automatically detect the connected video input signal(s) and apply the correct video mode and refresh rate.

4. DAILY OPERATION

4.1 Recommendations for daily operation

Optimize the lifetime of your display

Enabling the Display Power Management System (DPMS) of your display will optimize its diagnostic lifetime by automatically switching off the backlight when the display is not used for a specified period of time. By default, DPMS is enabled on your display, but it also needs to be activated on your workstation. To do this, go to “Power Options Properties” in the “Control Panel”.



Barco recommends setting DPMS activation after 20 minutes of non-usage.

Use a screen saver to avoid image retention

Prolonged operation of an LCD with the same content on the same screen area may result in a form of image retention.

You can avoid or significantly reduce the occurrence of this phenomenon by using a screen saver. You can activate a screen saver in the “Display properties” window of your workstation.



Barco recommends setting screen saver activation after 5 minutes of non-usage. A good screen saver displays moving content.

In case you are working with the same image or an application with static image elements for several hours continuously (so that the screen saver is not activated), change the image content regularly to avoid image retention of the static elements.

Understand pixel technology

LCD displays use technology based on pixels. As a normal tolerance in the manufacturing of the LCD, a limited number of these pixels may remain either dark or permanently lit, without affecting the diagnostic performance of the product. To ensure optimal product quality, Barco applies strict selection criteria for its LCD panels.



To learn more about LCD technology and missing pixels, consult the dedicated white papers available at www.barco.com/healthcare.

Enhance user comfort

Every Barco multi-head display system is color matched with the highest specifications in the market.



Barco recommends keeping color-matched displays together. Furthermore, it is important to use all displays of a multi-head configuration at the same rate to preserve color matching throughout the economic lifetime of the system.

Maximize quality assurance

The 'MediCal QAWeb' system offers online service for high-grade Quality Assurance, providing maximum diagnostic confidence and uptime.



Barco recommends to install MediCal QAWeb Agent and apply the default QAWeb policy at least. This policy includes calibration on regular intervals. Connecting to MediCal QAWeb Server offers even more possibilities.

Learn more and sign up for the free MediCal QAWeb Essential level at www.barco.com/healthcare/qa.

4.2 Key indicator lights

About the key indicator lights

By default, the indicator lights of the keys will be dimmed which makes the keys unavailable at that moment. To make the keys illuminate and available for further actions touch one of the keys. As a result, all keys will be illuminated and are now available for further actions. However, if no further actions are taken within the following 5 seconds, the keys will dim again.



The I-Luminate/Left key is always lit and available for activation of the I-Luminate feature. Please refer to "I-Luminate", page 27 for more information.




The key auto-dim function can be disabled in the OSD menus. Please refer to "Key indicator lights", page 30 for detailed instructions on how to do this.

4.3 Standby switching



The connected power supply also provides a switch that can be used to turn the power completely off. To use the display, please make sure to switch on this power supply. This can be done by pushing the on/off switch on the power supply into the "I" position.



To switch your display on using the keys:

Switching on the display while it is in standby mode can be done by:

1. Push the standby key once.

As a result, the display will switch on and the **power status indicator** light is **white**.



During start-up phase, the orange indicator light and the white indicator light are lit, until the unit is fully started.

To switch your display to Stand-by using the keys:

Switching off the display can be done by:

1. Push the standby key shortly for three times. After the second push, the OSD message "Power off" appears on the display, this means the display will go in standby mode.

As a result, the display will switch to stand-by mode and the **power status indicator** light is **orange**.



In case of a power outage recovery, your display will always start-up in the power mode it was in before the power interruption (i.e. stand-by or on). This protects your display against inadvertent image retention problems.

4.4 Bringing up the OSD menus

How to bring up the OSD menus

The OSD menu allows you to configure different settings to make your Coronis Uniti fit your needs within your working environment. Also, you can retrieve general information about your display and its current configuration settings through the OSD menu.

Bringing up the OSD menus can be done by:

1. If not already done so, switch on the display as previously described.
2. Illuminate the keys as previously described.
3. While the keys are illuminated, touch the menu key.

As a result, the OSD main menu comes up in the bottom right corner of the screen. However, if no further actions are taken within the following 90 seconds, the OSD will disappear again.



The OSD menu auto-exit function can be disabled in the OSD menu. Please refer to "OSD menu automatic close function", page 29 for detailed instructions on how to do this.

4.5 Navigating through the OSD menus

How to navigate through the OSD menus

Navigating through the OSD menus can be done by:

- Use the left/right keys to move through the (sub)menus, change values or make selections.
- To go into a submenu or confirm adjustments and selections, use the menu key.
- Use the standby key to cancel adjustments or exit a (sub)menu.
- Exit all OSD menus at once by touching the standby key for approximately 2 seconds.



The key icons are displayed above the keys, adapted to the function that it is used for (menu dependent).



I-Luminate is not available while the OSD menu is activated.

Overview key icons



Left, Right



Menu



Enter



Cancel



Standby (IEC 60417-5009)

4.6 Overview of the functionality of the Left/Right keys

Overview

Left key	Right key	Behavior			
Push	Push	Cycle viewing mode between text, diagnostic			
Push	No Push	Toggle on I-Luminate			
		Left key	Right key	Menu	Behavior
		Push	No push	No menu	Toggle off I-Luminate
		No push	Push	No menu	Cycle I-Luminate modes between text small film, large film, no film
		Push	Push	No menu	Cycle viewing mode between text and diagnostic, also toggle off I-Luminate
		No push	No push	Menu	Nothing

Left key	Right key	Behavior			
No Push	Push	Enable OSD			
		Left key	Right key	Menu	Behavior
		No push	Push	No menu	Cycle SoftGlow modes between task light, wall light, both, none.
		Push	No push	No menu	Nothing
		Push	Push	No menu	Cycle viewing mode between text and diagnostic
		No push	No push	Menu	Enter the OSD menu

4.7 I-Luminate

About I-Luminate

When the display is in power on mode and the OSD menu is not shown, I-Luminate can be activated by touching the I-luminate/left key.

When touching the I-Luminate key, the display will enter the I-Luminate mode, for approximately 1 minute. Touch the I-Luminate key again to immediately switch back to normal mode.

4.8 Extended display keypad functions

About extended display keypad functions

The concept of the extended display keypad functions is to present a selection of functions immediately available to the user without the need to navigate through the OSD Menu.



The extended display keypad functions will only be available when no OSD menu is visible on the screen.

4.8.1 I-luminate mode

To quickly change the I-luminate mode

1. While no OSD menu is on the screen, press the I-luminate/Left key to bring up the I-luminate quick selection menu.
2. Toggle the available I-luminate modes (see "I-Luminate default mode", page 32) by pressing the Right key.

4.8.2 Viewing mode

To quickly change the viewing mode

1. While no OSD menu is on the screen, press the Left key and Right key simultaneously to change the viewing mode.
2. Toggle the available viewing modes (see "Viewing modes", page 34) by pressing the Left/Right key simultaneously.

5. ADVANCED OPERATION

5.1 OSD menu language

About the OSD menu language

By default, the OSD menu comes up in English. However, there's a wide range of other languages available for the OSD menu of your Coronis Uniti.

To change the language of the OSD menu:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > User Interface > Menu* menu.
3. Enter the *Language* submenu.
4. Select one of the available languages and confirm.

5.2 OSD menu automatic close function

About the OSD menu automatic close function

By default, the OSD menu will disappear automatically after approximately 90 seconds of inactivity. However, this function can be disabled so that the OSD menu remains on the screen until manually closed.

To enable/disable the OSD menu automatic close function:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > User Interface > Menu* menu.
3. Enter the *Automatic Close* submenu.
4. Select *Enabled/Disabled* as desired and confirm.

5.3 Power status indicator light

About the power status indicator light

By default, when the display is switched on, the power status indicator light is dimmed. This behavior can be changed so that the power status indicator light will be **white** when the display is switched on.



When the display is in stand-by mode, the power status indicator light will always turn orange, even when the power status indicator light is disabled.

To enable/disable the power status indicator light:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > User Interface > Indicator Lights* menu.
3. Enter the *Power Status* submenu.
4. Select *Enabled/Disabled* as desired and confirm.

5.4 Key indicator lights

About the key indicator lights

By default, after lighting up, the key indicator lights will dim again if no further actions are taken within the following 5 seconds. However, this behavior can be changed so that the key indicator lights are always on or always off.

To configure the key indicator lights

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > User Interface > Indicator Lights* menu.
3. Enter the *Keys* submenu.
4. Select *Automatic/Always On/Always Off* as desired and confirm.

5.5 Power lock function

About the power lock function

By enabling the power lock function, the Coronis Uniti is forced to remain switched on. This means that it can't be switched to stand-by mode manually until the power lock function is disabled again.

To enable/disable the power lock function:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > User Interface > Controls* menu.
3. Enter the *Power Lock* submenu.
4. Select *Enabled/Disabled* as desired and confirm.

5.6 SoftGlow Task light

About the SoftGlow Task light

The Coronis Uniti is equipped with a SoftGlow Task light. This allows you to have light on your desk in a dark environment. The brightness of the SoftGlow Task light can be adjusted.

To enable/disable the SoftGlow Task light:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Lights* menu.
3. Enter the *SoftGlow Task light* submenu.
4. Select *Enabled/Disabled* as desired and confirm.

To adjust the SoftGlow Task light brightness:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Lights* menu.
3. Enter the *SoftGlow Task light brightness* submenu.
4. Set a *SoftGlow Task light brightness* value as desired and confirm.

5.7 SoftGlow Wall light

About the SoftGlow Wall light

The Coronis Uniti is equipped with a SoftGlow Wall light. This allows you to have light on the wall at the back of your display in a dark environment. The brightness of the SoftGlow Wall light can be adjusted.

To enable/disable the SoftGlow Wall light:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Lights* menu.
3. Enter the *SoftGlow Wall light* submenu.
4. Select *Enabled/Disabled* as desired and confirm.

To adjust the SoftGlow Wall light brightness:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Lights* menu.
3. Enter the *SoftGlow Wall light brightness* submenu.
4. Set a *SoftGlow Wall light brightness* value as desired and confirm.

5.8 DPMS mode

About DPMS mode

Enabling the Display Power Management System (DPMS) mode on your display will optimize its diagnostic lifetime by automatically switching off the backlight when the display is not used for a specified period of time. By default, DPMS mode is enabled on your display, but it also needs to be activated on your workstation. To do this, go to the "Power options properties" window of your workstation.



Barco recommends setting DPMS activation after 20 minutes of non-usage.



When DPMS mode is enabled on your display, an additional OSD power saving function becomes available: hibernate. Please refer to "Hibernate", page 32 for more information on hibernation and how to enable this function.

To enable/disable DPMS mode on your display:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Power Management* menu.
3. Enter the *DPMS Mode* submenu.
4. Select *Enabled/Disabled* as desired and confirm.

5.9 Hibernate

About hibernate

Enabling hibernation will not only switch off the backlight but will also force the display to disable other functionalities so that power consumption is further reduced to a minimum. This happens after a specific period of time which can be manually adjusted.



Hibernate can only be enabled on your display when the DPMS mode is enabled first. Therefore, please refer to "DPMS mode", page 31 to do this.

To enable/disable hibernation on your display:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Power Management* menu.
3. Enter the *Hibernate* submenu.
4. Select *Enabled/Disabled* as desired and confirm.

To specify the hibernate timeout:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Power Management* menu.
3. Enter the *Hibernate Timeout* submenu.
4. Set the timeout value as desired and confirm.

5.10 I-Luminate default mode

About the I-Luminate default mode

The I-Luminate mode defines the default activated mode during the I-Luminate boost. This mode can be:

Screen	The boost mode is applied on the screen display.
Film (large or small)	Film (large or small): the boost mode activates a high illuminated rectangle on top of the screen, simulating a light box for use with radiological film. The size of this rectangle is similar to a classic (large or small) radiological film.

To set the I-Luminate mode:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > I-Luminate* menu.
3. Enter the *Default mode* submenu.
4. Select *Screen/Small Film/Large Film* as desired and confirm.

5.11 I-Luminate film position

About the I-Luminate film position

By default, the I-Luminate rectangle comes up in the top/center of the left part of the screen. This position can be changed to top/left or top/right corner of the left part of the screen or top/left, top/center or top/right corner of the right part of the screen.

To set the I-Luminate film position:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > I-Luminate* menu.
3. Enter the *Film Position* submenu.
4. Select *Left Side Top Left/Center/Right* or *Right Side Top Left/Center/Right* as desired and confirm.

5.12 Luminance target

About the luminance target

The luminance target of your Coronis Uniti is adjustable over a predefined range. When you change the luminance target, the display will adjust its backlight to reach the target.

To set the luminance target:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Calibration* menu.
3. Enter the *Luminance Target* submenu.
4. Set a luminance target value as desired and confirm.



The default, factory DICOM calibrated luminance value is available in the technical specifications table. The guaranteed backlight lifetime is valid for this setting.

5.13 Color presets

About color presets

The available color preset settings for your display are:

Clearbase	Simulation of the clearbase film color temperature.
Bluebase	Simulation of the bluebase film color temperature.
User	When selecting the User color temperature setting, you will be able to manually define the X and Y coordinates or the display color temperature in separate submenus.
Native White	The native, unmodified color temperature of the LCD panel.

To select a color preset:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Calibration > Color Settings* menu.

3. Enter the *Color Presets* submenu.
4. Select one of the available Color Presets and confirm.

5.14 Color temperature

About color temperature:

It is possible to change the color temperature of your display.



Color temperature can only be changed on your display when color presets is set to user. Therefore, please refer to "Color presets", page 33 to do this.

To change the color temperature:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Calibration > Color Settings* menu.
3. Enter the *Color Definition* submenu.
4. Select Color Temperature and confirm.
5. Enter the *Color Temperature* submenu.
6. Set the Temperature value as desired and confirm.

5.15 Color coordinates

About color coordinates:

It is possible to change the color coordinates of your display.



Color coordinates can only be changed on your display when color presets is set to user. Therefore, please refer to "Color presets", page 33 to do this.

To change the color coordinates:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Calibration > Color Settings* menu.
3. Enter the *Color Definition* submenu.
4. Select Color Coordinates and confirm.
5. Enter the *x and/or y* submenu.
6. Set the coordinate value for x and/or y as desired and confirm.

5.16 Viewing modes

About viewing modes

The Coronis Uniti can be used in two viewing modes:

Diagnostic	This mode provides the full calibrated luminance and is intended for using the display for diagnostic purposes.
Text	In this mode, the luminance is reduced to approximately half of the luminance. This is intended for using the display with office applications such as word processing. Please note that text mode is not persistent, once powered off, the unit will restart in diagnostic mode.



To quickly switch the viewing mode without having to enter the OSD menu, touch the left and right key (the two leftmost buttons) at the same time during normal operation.



As the Coronis Uniti is intended to be used in a diagnostic environment, the diagnostic mode should always be selected.

To select a viewing mode:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Calibration* menu.
3. Enter the *Viewing Mode* submenu.
4. Select *Diagnostic/Text* as desired and confirm.

5.17 Display functions

About display functions

Native, uncorrected panels will display all grayscale/color levels with luminance increments that are not optimal for crucial diagnostic information. Studies have shown however, that in medical images certain grayscale/color parts contain more diagnostic information than others. To respond to these conclusions, display functions have been defined. These functions emphasize on these parts containing crucial diagnostic information by correcting the native panel behavior.

Native	If you select Native, the native panel behavior will not be corrected.
Dynamic Gamma 1.8 Dynamic Gamma 2.2	These are gamma functions that are shifted to take into account the non-zero luminance of an LCD panel when driven with a "black" signal. They are especially useful in CT applications to improve the perception of low Hounsfield values.
DICOM	DICOM (Digital Imaging and Communications in Medicine) is an international standard that was developed to improve the quality and communication of digital images in radiology. In short, the DICOM display function results in more visible grayscales in the images. Barco recommends selecting the DICOM display function for most medical viewing applications.

User	This display function will be automatically selected when display functions are defined by MediCal QAWeb.
Gamma 1.8 Gamma 2.2	Select one of these display functions in case the display is to replace a CRT display with a gamma of 1.8 or 2.2 respectively.

To select a display function:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Calibration* menu.
3. Enter the *Display Function* submenu.
4. Select one of the available display functions and confirm.

5.18 Ambient Light Compensation (ALC)

About ALC



Ambient Light Compensation (ALC) can only be enabled on your display when the DICOM display function is selected. Therefore, please refer to "Display functions", page 35 to correctly set the display function.

When ALC is enabled, the DICOM display function will be recalculated taking a preset ambient light correction value into account. This value is determined by the selected reading room. Therefore, it is also important to select a realistic reading room when enabling ALC. This can be done by following the instructions in "Reading rooms", page 36.

To enable/disable ALC:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Calibration > Ambient Light* menu.
3. Enter the *Ambient Light Compensation* submenu.
4. Select *Enabled/Disabled* as desired and confirm.

5.19 Reading rooms

About reading rooms



Reading rooms can only be selected when the DICOM display function is selected. Therefore, please refer to "Display functions", page 35 to correctly set the display function.

The American Association of Physicists in Medicine (AAPM) composed a list of pre-defined reading rooms. Each of these reading rooms are defined by following parameters:

- the maximum light allowed in this type of room
- the preset ambient light correction value for this reading room

These parameters are stored in your display and determine the preset ambient light correction value to take into account to recalculate the DICOM display function when Ambient Light Compensation (ALC) is enabled. Please refer to "Ambient Light Compensation (ALC)", page 36 to enable ALC.

The available reading rooms for your Coronis Uniti are:

CR/DR/ MAMMO	Corresponds to light conditions in diagnostic reading rooms for computed radiology, digital radiology or mammography. This setting has the lowest maximum ambient light.
CT/MR/NM	Corresponds to light conditions in diagnostic reading rooms for computed tomography, magnetic resonance or nuclear medicine scans.
Staff Office	Corresponds to light conditions in office rooms.
Clinical Viewing Room	Corresponds to light conditions in diagnostic reading rooms for clinical viewing.
Emergency Room	Corresponds to light conditions in emergency rooms.
Operating Room	Corresponds to light conditions in operating rooms. This setting has the highest maximum ambient light.

To select a reading room:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Calibration > Ambient Light* menu.
3. Enter the *Reading Room* submenu.
4. Select one of the available reading rooms and confirm.

5.20 Continuous ALC

About Continuous ALC



Continuous ALC can only be selected when the DICOM display function is selected. Therefore, please refer to "Display functions", page 35 to correctly set the display function.

Enabling continuous ALC will continuously recalculate the DICOM display function taking the averaged ambient light into account.

To select continuous ALC:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Calibration > Ambient Light* menu.
3. Enter the *Continuous ALC* submenu.
4. Select *Enabled/Disabled* as desired and confirm.

5.21 Embedded QA

Overview

- About Embedded QA
- DICOM status report
- DICOM compliance check
- DICOM calibration
- Reset DICOM calibration

- DICOM error threshold

5.21.1 About Embedded QA

About

Embedded QA allows you to run a display calibration or compliance test directly from the display using the OSD menus described in the next sections. Embedded QA will use the front sensor / I-Guard to measure the necessary luminance levels for either a calibration or compliance test. Various settings for both actions can be selected from the display's OSD menu. The last results of both actions can be consulted from the OSD.

Embedded QA or MediCal QAWeb?

Embedded QA is not a replacement for the Barco MediCal QAWeb solution.

Although Embedded QA is a reliable option to perform a simple calibration or compliance test, Barco still highly recommends MediCal QAWeb as the solution of choice for calibration and QA. Medical QAWeb brings many benefits such as centralized asset management, the ability to schedule tasks, remote management, automated reporting, alerting and specific support of regional QA standards such as DIN 6868-57, JESRA and AAPM TG18. That's why MediCal QAWeb Agent acts as the master for all supported displays from the moment it is installed and running. MediCal QAWeb Agent will take over from Embedded QA and overwrite any settings which were applied by Embedded QA.

5.21.2 DICOM status report

About DICOM status report

Following information is available:

DICOM Compliance Status (status since last compliance check)	Compliance status	Shows if the current DICOM curve is compliant or not.
	Maximum error	Shows the maximum error of the current DICOM curve. This is the deviation compared to a perfect DICOM.
	Error threshold	Shows the error threshold. This is the maximum error allowed before a DICOM calibration is required.
	Time elapsed since latest compliance check	Shows the backlight runtime since last compliance check.
	Display Function	Shows the current display function.
	Ambient light compensation	Shows the ambient light compensation status.
	Reading Room	Shows the selected reading room.
	Luminance	Shows the measured luminance.
	Black luminance	Shows the measured backlight luminance.
DICOM Calibration Status	No calibration executed yet.	No other information is visible
	Calibration executed.	When the calibration is executed, the following extra information is shown: Backlight runtime elapsed since latest calibration, display function, ambient light compensation, reading room.

Current DICOM Settings	Display function	Shows the current display function.
	Ambient Light Compensation	Shows the ambient light compensation status.
	Reading room	Shows the selected reading room.

To retrieve the DICOM status report:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Calibration > Embedded QA* menu.
3. Select *DICOM status report* to make the information visible on the screen.

5.21.3 DICOM compliance check**About DICOM compliance check**

The DICOM compliance check will measure the DICOM curve of your display in different steps. After measurement, the DICOM status report is shown.

To start DICOM compliance check:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Calibration > Embedded QA* menu.
3. Select *DICOM compliance check* to start the compliance check.
Warning: Pressing a key during the compliance check will abort the check.

5.21.4 DICOM calibration**About DICOM calibration**

The DICOM calibration will add a correction to the current DICOM curve to approach the perfect DICOM curve as good as possible.

To start DICOM calibration:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Calibration > Embedded QA* menu.
3. Select *DICOM calibration* to start the calibration.
Warning: Pressing a key during calibration will abort the calibration, previous values will be restored.
Note: After calibration, the compliance check will start automatically.

5.21.5 Reset DICOM calibration**About reset DICOM calibration**

It is possible to restore the original (not corrected) DICOM curve.

To reset the DICOM calibration:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Calibration > Embedded QA* menu.
3. Enter the *DICOM preferences* submenu.
4. Select *reset DICOM calibration* to restore the original (not corrected) DICOM curve.

5.21.6 DICOM error threshold

About DICOM error threshold

The threshold to define the DICOM compliance can be modified in steps of 5% starting from 5 to 30%. When the maximum deviation is not bigger than the selected threshold, the compliance check will be OK.

To set the DICOM error threshold:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Calibration > Embedded QA* menu.
3. Enter the *DICOM preferences* submenu.
4. Set *DICOM error threshold* as desired and confirm.

5.22 Image scaling

About image scaling

Enabling image scaling will multiply each individual pixel to one or more adjacent pixels so that the size of the displayed image will be a multiple of the original image source video input signal.



Image scaling is only possible when the resolution of your display's video input signal is less than or equal to half the maximum resolution of the display.

To enable/disable image scaling:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Image Source* menu.
3. Enter the *Scaling* submenu.
4. Select *Enabled/Disabled* as desired and confirm.

5.23 Image source selection modes

About image source selection modes

Your Coronis Uniti automatically detects the number of video input signals connected, attaches them to the correct display side and applies the correct video settings to it (resolution, video encoding mode, refresh rate,...). However, it may be needed to manually select the video input signal(s) to be displayed on a certain display side or to adjust certain video settings yourself. The start to this is selecting one of the following image source selection modes available for your display:

Automatic	In this mode, your display automatically detects the connected video input signals, attaches them to the correct display side and applies the correct video settings to it (resolution, video encoding mode, refresh rate,...). No video settings are available when this mode is selected.
One Image Source	This mode is intended for displaying and manually configuring only one connected video input signal. When selecting this mode, the video settings become available for the selected video input signal.

Two Image Sources	This mode is intended for displaying and manually configuring two connected video input signals (one on each display side). When selecting this mode, the video settings become available for the selected video input signal on each side of the display.
Expert mode	This mode is intended for displaying and manually configuring one or two connected video input signals. When selecting this mode, the video settings become available for both video input signals on both sides of the display.

To select an image source selection mode:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Image Sources* menu.
3. Enter the *Image Source Selection* submenu.
4. Select one of the available image source selection modes and confirm.

5.24 Grayscale conversion modes

About grayscale conversion modes

Grayscale conversion modes specify how color generated on the display controller is converted to grayscale in your display.

The available grayscale conversion modes are:

No Conversion	
Use Red Channel	This mode is intended for grayscale displays where gray is sent over the red channel.
Use Green Channel	This mode is intended for grayscale displays where gray is sent over the green channel.
Use Blue Channel	This mode is intended for grayscale displays where gray is sent over the blue channel.

To manually select a grayscale conversion mode:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Image Sources > Input Settings > DisplayPort1/2* menu.
3. Enter the *Grayscale Conversion* submenu.
4. Select one of the available color conversion modes and confirm.

5.25 Input interface standard version

About Input interface standard version

The Coronis Uniti supports two input interface standard versions: DPCD V1.1 and DPCD V1.2

To select the EDID format

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Image Sources > Input Settings > DisplayPort1/2* menu.
3. Enter the *Input interface standard version* submenu.

4. Select one of the available versions and confirm.



To obtain full resolution (2100 x 2800) and full refresh rate (60Hz), DPCD V1.2 should be selected.

5.26 EDID format

About EDID format

The Coronis Uniti supports two EDID formats: E-EDID V1.4 and DisplayID V1.3

To select the EDID format

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Image Sources > Input Settings > > DisplayPort 1/2 > EDID* menu.
3. Enter the *EDID format* submenu.
4. Select one of the available format and confirm.

5.27 EDID timings

About EDID timings

Following EDID timings are available for your Coronis Uniti:

Refresh Rate	Allows to manually select the refresh rate of the image source video input signal depending on the maximum refresh rate of the display controller connected to your display.
Preferred Orientation	Allows to change the orientation of the image source video input signal to landscape, portrait or to let the display automatically assign the correct orientation.
Color Depth	Allows to change the color depth to 8 or to 10 bit.

To manually set EDID timings:

1. Bring up the OSD main menu.
2. Navigate to the *Configuration > Image Sources > Input Settings > DisplayPort 1/2* menu.
3. Enter the *EDID* submenu.
4. Select *Resolution, Refresh Rate, Preferred Orientation* or *Color Depth*.
5. Select one of the available settings and confirm.

5.28 Display info

About display info

Your display serial number, color type, native resolution, firmware versions, etc. are available in a dedicated submenu of the OSD menu.

To retrieve info about your display:

1. Bring up the OSD main menu.
2. Navigate to the *About this Display* menu to make the information visible on the screen.

5.29 Display status

About display status

The Status submenu of the OSD menu provides info on the current status of your display (runtimes, temperatures, etc.), the status of the connected image sources (video encoding mode, timings, etc.), the current calibration status of your display (display function, luminance, ALC, etc.) and the status about activated connections.

To retrieve the status of your display:

1. Bring up the OSD main menu.
2. Navigate to the *Status* menu.
3. Enter the *Display*, *Image Sources*, *Calibration* or *Connectivity* submenu as desired.

6. CLEANING YOUR DISPLAY

6.1 Cleaning instructions

To clean the display

Clean the display using a sponge, cleaning cloth or soft tissue, lightly moistened with a recognized cleaning product for medical equipment. Read and follow all label instructions on the cleaning product. In case of doubt about a certain cleaning product, use plain water.

Do not use following products:

- Alcohol/solvents at higher concentration > 5%
- Strong alkalis lye, strong solvents
- Acid
- Detergents with fluoride
- Detergents with ammonia
- Detergents with abrasives
- Steel wool
- Sponge with abrasives
- Steel blades
- Cloth with steel thread



CAUTION: Take care not to damage or scratch the front glass or LCD. Be careful with rings or other jewelry and do not apply excessive pressure on the front glass or LCD.



CAUTION: Do not apply or spray liquid directly to the display as excess liquid may cause damage to internal electronics. Instead, apply the liquid to a cleaning cloth.

7. IMPORTANT INFORMATION

7.1 Safety information

General recommendations

Read the safety and operating instructions before operating the device.

Retain safety and operating instructions for future reference.

Adhere to all warnings on the device and in the operating instructions manual.

Follow all instructions for operation and use.

Electrical Shock or Fire Hazard

To prevent electric shock or fire hazard, do not remove cover.

No serviceable parts inside. Refer servicing to qualified personnel.

Do not expose this apparatus to rain or moisture.

Modifications to the unit:

Do not modify this equipment without authorization of the manufacturer.

Type of protection (electrical):

Display with external power supply: Class I equipment.

Degree of safety (flammable anesthetic mixture):

Equipment not suitable for use in the presence of a flammable anesthetic mixture with air or with oxygen or nitrous oxide.

Non-patient care equipment

- Equipment primarily for use in a health care facility that is intended for use where contact with a patient is unlikely (no applied part).
- The equipment may not be used with life support equipment.
- The user should not touch the equipment, nor its signal input ports (SIP)/signal output ports (SOP) and the patient at the same time.

Power connection – Equipment with external 24 VDC power supply

- Power requirements: The equipment must be powered using the delivered medical approved 24 VDC (≡) SELV power supply.
- The medical approved DC (≡) power supply must be powered by the AC mains voltage.
- The power supply is specified as a part of the ME equipment or combination is specified as a ME system.
- To avoid the risk of electric shock, this equipment must only be connected to a supply mains with protective earth.
- The equipment should be installed near an easily accessible outlet.
- The equipment is intended for continuous operation.

Transient over-voltage

If the device is not used for a long time, disconnect it from the AC inlet to avoid damage by transient over-voltage.

7. Important information

To fully disengage the power to the device, please disconnect the power cord from the AC inlet.

Power cords:

- Do not overload wall outlets and extension cords as this may result in fire or electric shock.
- Mains lead protection (U.S.: Power cord): Power cords should be routed so that they are not likely to be walked upon or pinched by items placed upon or against them, paying particular attention to cords at plugs and receptacles.
- The power supply cord should be replaced by the designated operator only at all time.
- Use a power cord that matches the voltage of the power outlet, which has been approved and complies with the safety standard of your particular country.

Water and moisture

Never expose the device to rain or moisture.

Never use the device near water - e.g. near a bathtub, washbasin, swimming pool, kitchen sink, laundry tub or in a wet basement.

Ventilation

Do not cover or block any ventilation openings in the cover of the set. When installing the device in a cupboard or another closed location, heed the necessary space between the set and the sides of the cupboard.

Installation

Place the device on a flat, solid and stable surface that can support the weight of at least 3 devices. If you use an unstable cart or stand, the device may fall, causing serious injury to a child or adult, and serious damage to the device.

This apparatus conforms to:

IEC 60950-1:2005 + C1:2006 + A1:2009 + C1:2012 + A2:2013, EN 60601-1:2007 + A11:2011, IEC 60601-1:2005 + A1:2012, ANSI/AAMI ES 60601-1:2005 + A1:2012, CAN/CSA C22.2 No. 60601-1:2014

IEC 60601-1-2:2007, EN 60601-1-2: 2007 + AC: 2010, FCC Class B, ICES-001 Class B, VCCI Class A



WARNING: VCCI Class A

この装置は、クラス A 情報技術装置です。この装置を家庭環境で使用すると電波妨害を引き起こすことがあります。この場合には使用者が適切な対策を講ずるよう要求されることがあります。

National Scandinavian Deviations for CL. 1.7.2:

Finland: "Laitte on liitettävä suojamaadoituskoskettimilla varustettuun pistorasiaan"

Norway: "Apparatet må tilkoples jordet stikkontakt"

Sweden: "Apparaten skall anslutas till jordat uttag"

7.2 Environmental information

Disposal Information

Waste Electrical and Electronic Equipment



■ This symbol on the product indicates that, under the European Directive 2012/19/EU governing waste from electrical and electronic equipment, this product must not be disposed of with other municipal

waste. Please dispose of your waste equipment by handing it over to a designated collection point for the recycling of waste electrical and electronic equipment. To prevent possible harm to the environment or human health from uncontrolled waste disposal, please separate these items from other types of waste and recycle them responsibly to promote the sustainable reuse of material resources.

For more information about recycling of this product, please contact your local city office or your municipal waste disposal service.

For details, please visit the Barco website at: <http://www.barco.com/en/AboutBarco/weee>

Turkey RoHS compliance



■ Türkiye Cumhuriyeti: AEEE Yönetmeliğine Uygundur.

[Republic of Turkey: In conformity with the WEEE Regulation]

中国大陆 RoHS

Chinese Mainland RoHS

根据中国大陆《电子信息产品污染控制管理办法》(也称为中国大陆RoHS), 以下部分列出了Barco产品中可能包含的有毒和/或有害物质的名称和含量。中国大陆RoHS指令包含在中国信息产业部MCV标准: “电子信息产品中有毒物质的限量要求”中。

According to the “China Administration on Control of Pollution Caused by Electronic Information Products” (Also called RoHS of Chinese Mainland), the table below lists the names and contents of toxic and/or hazardous substances that Barco’s product may contain. The RoHS of Chinese Mainland is included in the MCV standard of the Ministry of Information Industry of China, in the section “Limit Requirements of toxic substances in Electronic Information Products”.

零件项目(名称) Component name	有毒有害物质或元素 Hazardous substances and elements					
	铅 Pb	汞 Hg	镉 Cd	六价铬 Cr6+	多溴联苯 PBB	多溴二苯醚 PBDE
印制电路配件 Printed Circuit Assemblies	x	o	o	o	o	o
液晶面板 LCD panel	x	o	o	o	o	o
外接电(线)缆 External Cables	x	o	o	o	o	o
内部线路 Internal wiring	o	o	o	o	o	o
金属外壳 Metal enclosure	o	o	o	o	o	o
塑胶外壳 Plastic enclosure	o	o	o	o	o	o
散热片(器) Heatsinks	o	o	o	o	o	o
电源供应器 Power Supply Unit	x	o	o	o	o	o
风扇 Fan	o	o	o	o	o	o

7. Important information

零件项目(名称) Component name	有毒有害物质或元素 Hazardous substances and elements					
	铅 Pb	汞 Hg	镉 Cd	六价铬 Cr6+	多溴联苯 PBB	多溴二苯醚 PBDE
文件说明书 Paper Manuals	0	0	0	0	0	0
光盘说明书 CD manual	0	0	0	0	0	0
O: 表示该有毒有害物质在该部件所有均质材料中的含量均在 SJ/T 11363-2006 标准规定的限量要求以下。 O: Indicates that this toxic or hazardous substance contained in all of the homogeneous materials for this part is below the limit requirement in SJ/T11363-2006.						
X: 表示该有毒有害物质至少在该部件的某一均质材料中的含量超出 SJ/T 11363-2006 标准规定的限量要求。 X: Indicates that this toxic or hazardous substance contained in at least one of the homogeneous materials used for this part is above the limit requirement in SJ/T11363-2006						

在中国大陆销售的相应电子信息产品(EIP)都必须遵照中国大陆《电子信息产品污染控制标识要求》标准贴上环保使用期限(EFUP)标签。Barco产品所采用的EFUP标签(请参阅实例,徽标内部的编号使用于制定产品)基于中国大陆的《电子信息产品环保使用期限通则》标准。

All Electronic Information Products (EIP) that are sold within Chinese Mainland must comply with the "Electronic Information Products Pollution Control Labeling Standard" of Chinese Mainland, marked with the Environmental Friendly Use Period (EFUP) logo. The number inside the EFUP logo that Barco uses (please refer to the photo) is based on the "Standard of Electronic Information Products Environmental Friendly Use Period" of Chinese Mainland.



7.3 Regulatory compliance information

Indications for use

The Coronis Uniti is intended to be used in displaying and viewing digital images, including standard and multi-frame digital mammography, for review, analysis and diagnosis by trained medical practitioners. It is especially designed for breast tomosynthesis applications.

Caution (USA): Federal law restricts this device to sale by or on the order of a physician or a practitioner trained on its use.

FCC class B

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

This device has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This device generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this device does cause harmful interference to radio or television reception, which can be determined by turning the device off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the device and receiver.
- Connect the device into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

Canadian notice

This ISM device complies with Canadian ICES-001.

Cet appareil ISM est conforme à la norme NMB-001 du Canada.

7.4 EMC notice

General information

No specific requirement on the use of external cables or other accessories except power supply.

With the installation of the device, use only the delivered power supply or a spare part provided by the legal manufacturer. Using another can result in a decrease of the immunity level of the device.

Electromagnetic emissions

The Coronis Uniti is intended for use in the electromagnetic environment specified below. The customer or the user of the Coronis Uniti should assure that it is used in such an environment.

Emissions test	Compliance	Electromagnetic environment – Guidance
RF emissions CISPR 11	Group 1	The Coronis Uniti uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class B	The Coronis Uniti is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
Harmonic emissions IEC 61000-3-2	Class D	
Voltage fluctuations/ flicker emissions IEC 61000-3-3	Complies	

This Coronis Uniti complies with appropriate medical EMC standards on emissions to, and interference from surrounding equipment. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Interference can be determined by turning the equipment off and on.

7. Important information

If this equipment does cause harmful interference to, or suffer from harmful interference of, surrounding equipment, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna or equipment.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced technician for help.


Electromagnetic immunity

The Coronis Uniti is intended for use in the electromagnetic environment specified below. The customer or the user of the Coronis Uniti should assure that it is used in such an environment.

Immunity test	IEC 60601 Test levels	Compliance level	Electromagnetic environment – guidance
Electrostatic discharge (ESD) IEC 61000-4-2	± 6kV contact ± 8kV air	± 6kV contact ± 8kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%
Electrical fast transient/burst IEC 61000-4-4	± 2kV for power supply lines ± 1kV for input/ output lines	± 2kV for power supply lines ± 1kV for input/ output lines	Mains power quality should be that of a typical commercial or hospital environment
Surge IEC61000-4-5	± 1 kV line(s) to line(s) ± 2 kV line(s) to earth	± 1 kV line(s) to line(s) ± 2 kV line(s) to earth	Mains power quality should be that of a typical commercial or hospital environment
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	< 5% U_T ($> 95\%$ dip in U_T) for 0.5 cycle 40% U_T (60% dip in U_T) for 5 cycles 70% U_T (30% dip in U_T) for 25 cycles < 5% U_T ($>95\%$ dip in U_T) for 5s	< 5% U_T ($> 95\%$ dip in U_T) for 0.5 cycle 40% U_T (60% dip in U_T) for 5 cycles 70% U_T (30% dip in U_T) for 25 cycles < 5% U_T ($>95\%$ dip in U_T) for 5s	Mains power quality should be that of a typical commercial or hospital environment. If the user of the Coronis Uniti requires continued operation during power mains interruptions, it is recommended that the Coronis Uniti be powered from an uninterruptible power supply or a battery.
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	3 A/m	Not applicable ²	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.
Conducted RF IEC 61000-4-6 Radiated RF IEC 61000-4-3	3 Vrms 150 kHz to 80 MHz 3 V/m 80 MHz to 2.5 GHz	3 V 3 V/m	Portable and mobile RF communications equipment should be used no closer to any part of the Coronis Uniti, including cables, than the recommended separation distance

1. is the a.c. mains voltage prior to application of the test level.

2. Coronis Uniti doesn't contain susceptible components to magnetic fields

Immunity test	IEC 60601 Test levels	Compliance level	Electromagnetic environment – guidance
			<p>calculated from the equation applicable to the frequency of the transmitter. Recommended separation distance</p> <p>$d = 1.2\sqrt{P}$</p> <p>$d = 1.2\sqrt{P}$ 80 MHz to 800 MHz</p> <p>$d = 2.3\sqrt{P}$ 800 MHz to 2.5 GHz</p> <p>Where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in meters (m).</p> <p>Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey,³ should be less than the compliance level in each frequency range.⁴</p> <p>Interference may occur in the vicinity of equipment marked with symbol:</p> 



At 80 MHz and 800 MHz, the higher frequency range applies.



These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

3. Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the Coronis Uniti is used exceeds the applicable RF compliance level above, the Coronis Uniti should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the Coronis Uniti.

4. Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.

Recommended separation distance

The Coronis Uniti is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the Coronis Uniti can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the Coronis Uniti as recommended below, according to the maximum output power of the communications equipment.

Rated maximum output power of transmitter ⁵ W	Separation distance according to frequency of transmitter		
	150kHz to 80MHz $d=1.2\sqrt{P}$	80MHz to 800MHz $d=1.2\sqrt{P}$	800MHz to 2.5GHz $d=2.3\sqrt{P}$
0.01	0.12	0.12	0.23
0.1	0.38	0.38	0.73
1	1.2	1.2	2.3
10	3.8	3.8	7.3
100	12	12	23



At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.







These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.
















7.5 Explanation of symbols

Symbols on the device

On the device or power supply, you may find the following symbols (nonrestrictive list):






	Indicates compliance with the Directive 93/42/EEC as Class I device
	Indicates compliance with the Directive 93/42/EEC as Class II device
	Indicates compliance with Part 15 of the FCC rules (Class A or Class B)
	Indicates the device is approved according to the UL regulations

⁵. For transmitters rated at a maximum output power not listed above, the recommended separation distance d in meters (m) can be estimated using the equation applicable to the frequency of the transmitter. Where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

	Indicates the device is approved according to the UL regulations for Canada and US
	Indicates the device is approved according to the UL Demko regulations
	Indicates the device is approved according to the CCC regulations
	Indicates the device is approved according to the VCCI regulations
	Indicates the device is approved according to the KC regulations
	Indicates the device is approved according to the BSMI regulations
	Indicates the device is approved according to the PSE regulations
	Indicates the USB connectors on the device
	Indicates the DisplayPort connectors on the device
	Indicates the manufacturing date
	Indicates the temperature limitations ⁶ for the device to safely operate within specs
	Indicates the device serial no.
	Warning: dangerous voltage
	Caution
	Consult the operating instructions

6. Values for xx and yy can be found in the technical specifications paragraph.

7. Important information

	Indicates this device must not be thrown in the trash but must be recycled, according to the European WEEE (Waste Electrical and Electronic Equipment) directive
	Indicates Direct Current (DC)
	Indicates Alternating Current (AC)
	Stand-by
	Equipotentiality

7.6 Legal disclaimer

Disclaimer notice

Although every attempt has been made to achieve technical accuracy in this document, we assume no responsibility for errors that may be found. Our goal is to provide you with the most accurate and usable documentation possible; if you discover errors, please let us know.

Barco software products are the property of Barco. They are distributed under copyright by Barco N.V. or Barco, Inc., for use only under the specific terms of a software license agreement between Barco N.V. or Barco Inc. and the licensee. No other use, duplication, or disclosure of a Barco software product, in any form, is authorized.

The specifications of Barco products are subject to change without notice.

Trademarks

All trademarks and registered trademarks are property of their respective owners.

Copyright notice

This document is copyrighted. All rights are reserved. Neither this document, nor any part of it, may be reproduced or copied in any form or by any means - graphical, electronic, or mechanical including photocopying, taping or information storage and retrieval systems - without written permission of Barco.

© 2014 Barco N.V. All rights reserved.

7.7 Technical specifications

Overview

Screen technology	IPS
Active screen size (diagonal)	853.44 mm (33.6")
Active screen size (H x V)	708.1 x 472.1 mm (27.8 x 18.6")
Aspect ratio (H:V)	3:2
Resolution	4200 x 2800
Pixel pitch	0.1686 mm

Color imaging	Yes
Gray imaging	Yes
Color support	Yes
Viewing angle (H, V)	178°, CR ≥ 10
Uniform Luminance Technology (ULT)	Color PPU
Per Pixel Uniformity (PPU)	Yes, in color
Ambient Light Compensation (ALC)	Yes
Backlight Output Stabilization (BLOS)	Yes
I-Guard	Yes
Maximum luminance	> 2100 cd/m ² (PPU on)
DICOM calibrated luminance (ULT off)	1000 cd/m ²
Contrast ratio (typical)	1200:1 (PPU on)
Response time (Tr + Tf)	< 33 ms
Scanning frequency	25 - 85 Hz
Housing color	RAL 9004 + RAL 9003
Video input signals	DP1.2
USB ports	4 (1 upstream, 3 downstream)
USB standard	2.0
Power requirements (nominal)	100 - 240 V
Power consumption (nominal)	190 W
Power save mode	Yes
Power management	VESA DPMS
Dot clock	195 MHz
OSD languages	English, German, French, Dutch, Italian, Spanish, Portuguese, Swedish, Chinese (simplified), Japanese, Korean, Arabic, Polish, Russian
Dimensions with stand (W x H x D)	795 x 610 x 300 mm (lowest position)
Dimensions w/o stand (W x H x D)	795 x 572 x 131 mm
Dimensions packaged (W x H x D)	960 x 715 x 395 mm
Net weight with stand	33 kg
Net weight w/o stand	24 kg
Net weight packaged with stand	42 kg
Net weight packaged w/o stand	N/A
Height adjustment range	95 mm
Tilt	-5° / +30°
Swivel	-23° / +23°
Pivot	N/A
Mounting standard	VESA (200 x 100 mm & 100 x 100 mm)
Screen protection	Protective, non-reflective glass cover
Recommended modalities	Radiology, mammography and digital breast tomosynthesis

7. Important information

Certifications	IEC 60950-1:2005 + C1:2006 + A1:2009 + C1:2012 + A2:2013, EN 60601-1:2007 + A11:2011, IEC 60601-1:2005 + A1:2012, ANSI/AAMI ES 60601-1:2005 + A1:2012, CAN/CSA C22.2 No. 60601-1:2014 IEC 60601-1-2:2007, EN 60601-1-2: 2007 + AC: 2010, FCC Class B, ICES-001 Class B, VCCI Class A
Supplied accessories	User Guide
	Quick Installation Sheet
	Video cables (2x DisplayPort)
	Main cables (UK, European (CEBEC/KEMA), USA (UL/ CSA; adaptor plug NEMA 5-15P), Chinese (CCC))
	USB 2.0 cable
	External power supply
	Film clip
	MultiTouchPad
Optional accessories	None
QA software	QAWeb
Units per pallet	6
Pallet dimensions (W x H)	1000 x 1200
Warranty	5 years, 40k hours backlight warranty
Operating temperature	+0°C / +35°C
Storage temperature	-20°C / +60°C
Operating humidity	20% - 85% RH
Storage humidity	5% - 85% RH
Operation altitude	max. 3000 m

7.8 Open source license information

Open source license information

Open source license usage

This product contains software components released under an Open Source license. A copy of the source code is available on request by contacting your Barco customer support representative.

EACH SEPARATE OPEN SOURCE SOFTWARE COMPONENT AND ANY RELATED DOCUMENTATION ARE PROVIDED "AS IS" WITHOUT EXPRESS OR IMPLIED WARRANTY INCLUDING, BUT NOT LIMITED TO, THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE. IN NO EVENT SHALL THE COPYRIGHTHOLDER OR ANY OTHER CONTRIBUTOR BE LIABLE FOR DIRECT, INCIDENTAL OR CONSEQUENTIAL DAMAGES, EVEN IF ADVISED OF THE POSSIBILITY OF SUCH DAMAGES. MORE INFORMATION/DETAILS IS TO BE FOUND IN EACH SPECIFIC OPEN SOURCE LICENSE.

Copyright on each Open Source Software component belongs to the respective initial copyright holder, each additional contributor and/or their respective assignee(s), as may be identified in the respective documentation, source code, README file, or otherwise. You shall not remove or obscure or otherwise alter the respective copyrights.

You acknowledge living up to the conditions of each separate Open Source Software license.

A list of the Open Source Software components used is available in the applicable EULA, through the (customer section of the) Barco website or through other (online) means.